


PREPARATION OF EXPANDED, SINTERED PTFE BASE GRAFT

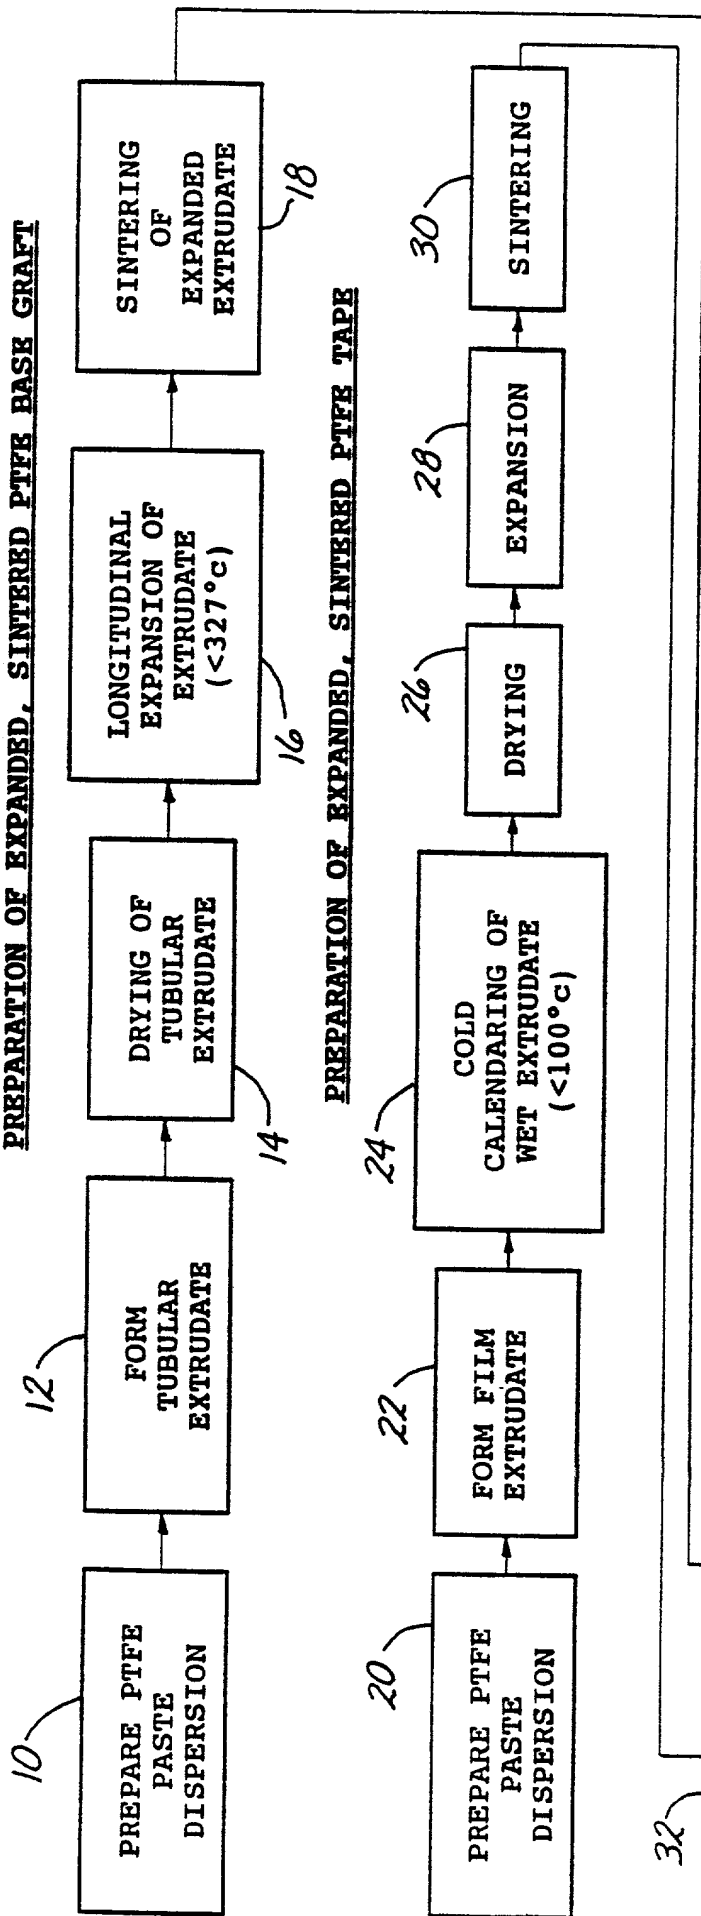

PREPARATION OF EXPANDED, SINTERED PTFE TAPE



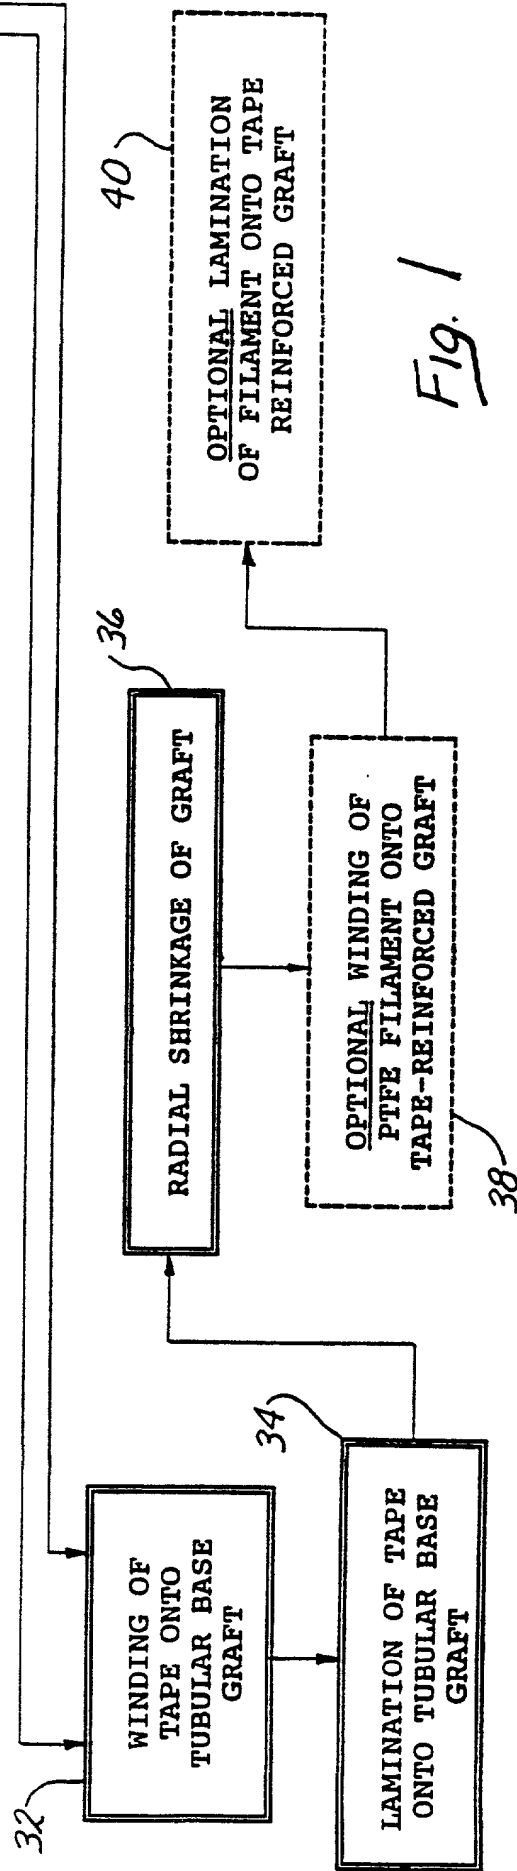


Fig. 1

PREPARATION OF SMALL DIAMETER EXPANDED, SINTERED PTFE BASE GRAFT

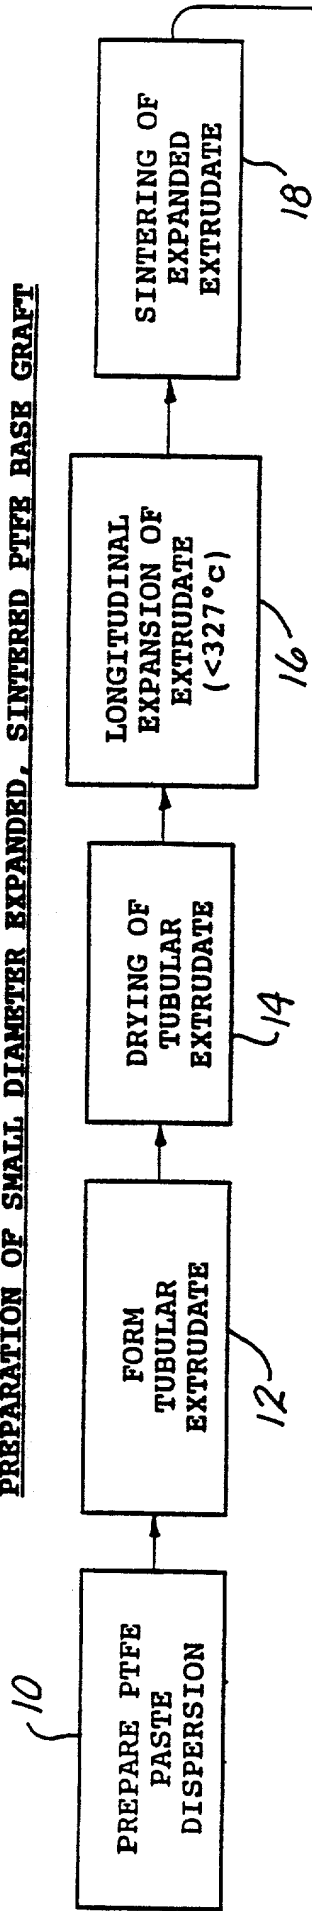

PREPARATION OF EXPANDED, SINTERED PTFE TAPE

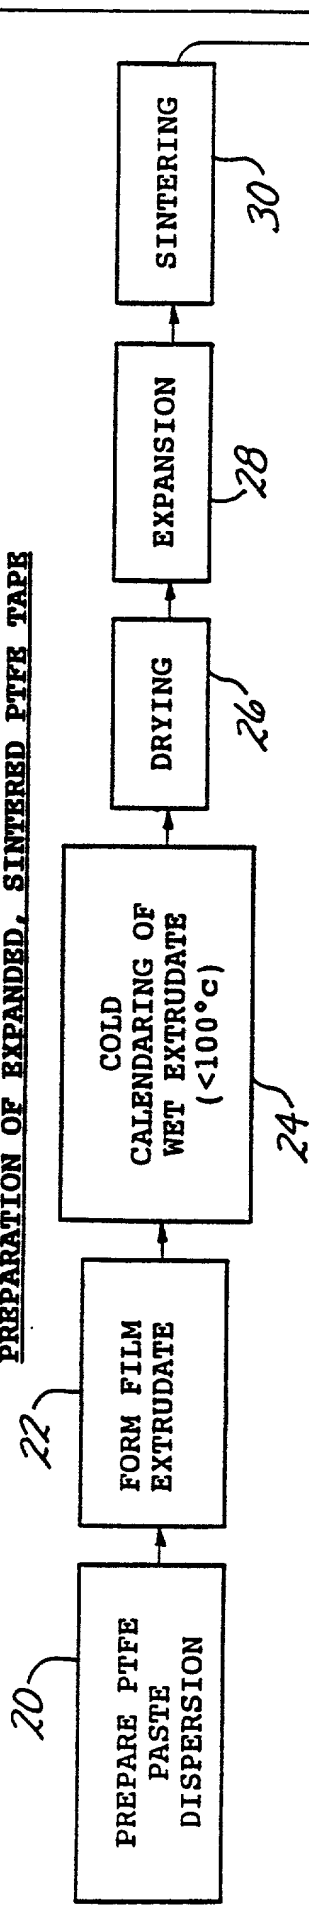

PREPARATION OF RADIALLY ENLARGEABLE TAPE-REINFORCED GRAFT

PREPARATION AND SHRINKAGE OF TAPE-TUBE

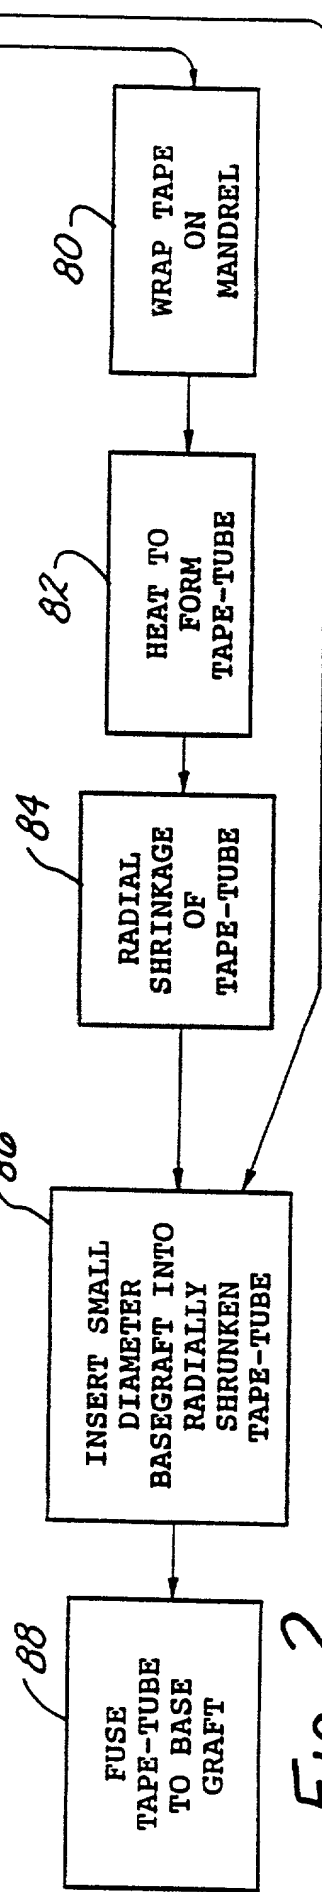


Fig. 2

ENDOASCULAR PLACEMENT AND IN SITU POST-EXPANSION OF RADIALLY-ENLARGEABLE,

TAPE-REINFORCED, TUBULAR GRAFT

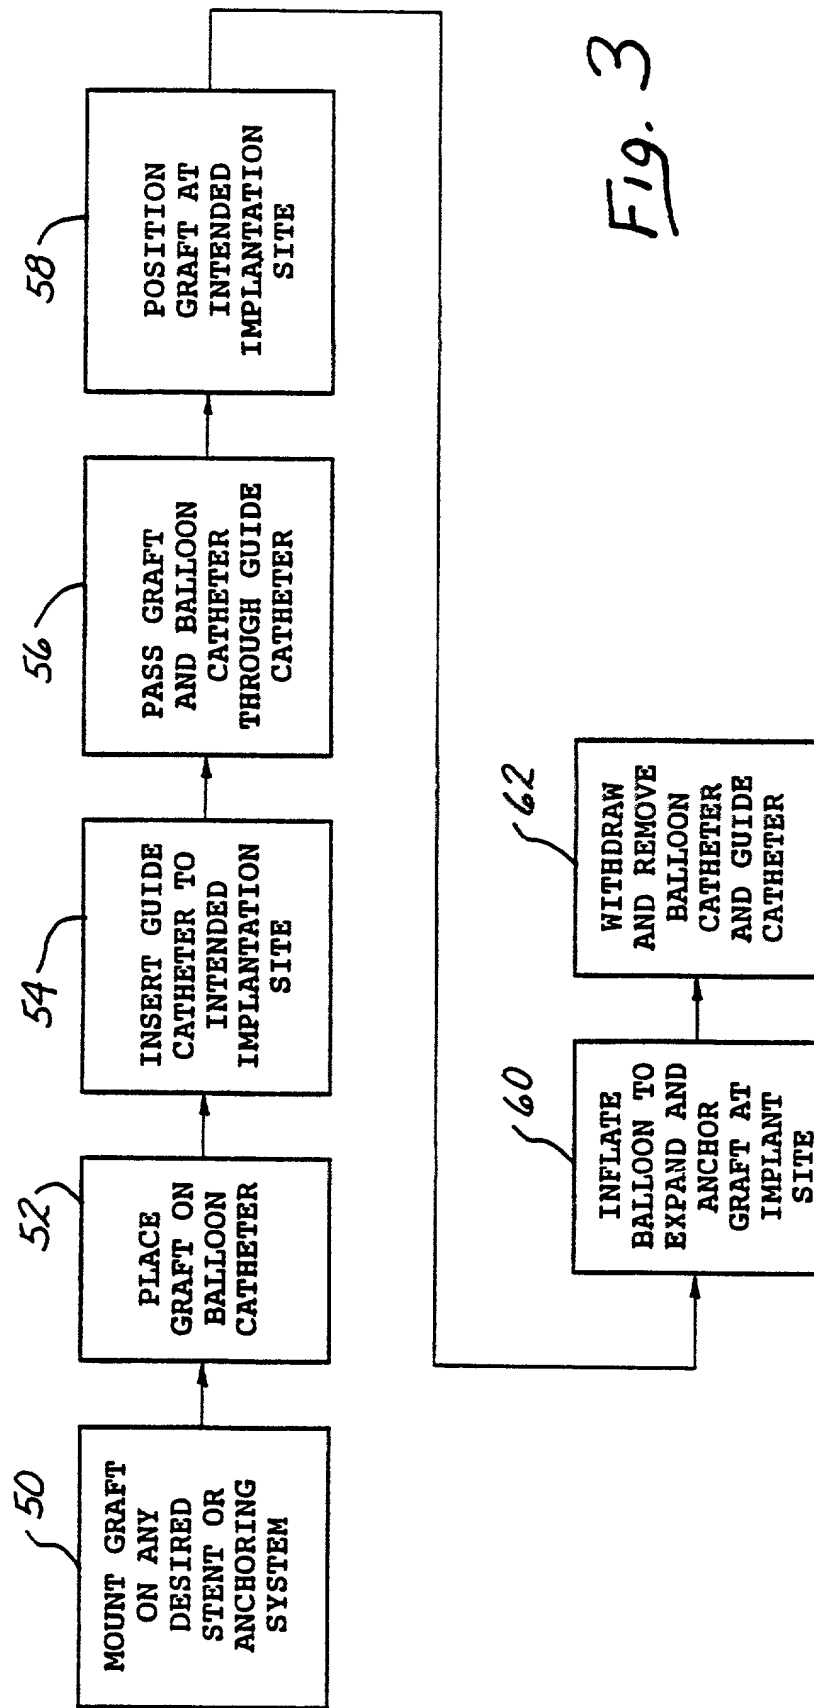


Fig. 3